

Sample Name :EGF Receptor Substrate 2 (Phospho-Tyr5)
 Cat No.: RP20109
 Lot No.: E5579319J
 Time Processed :4:33:35
 Month-Day-Year Processed :10/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

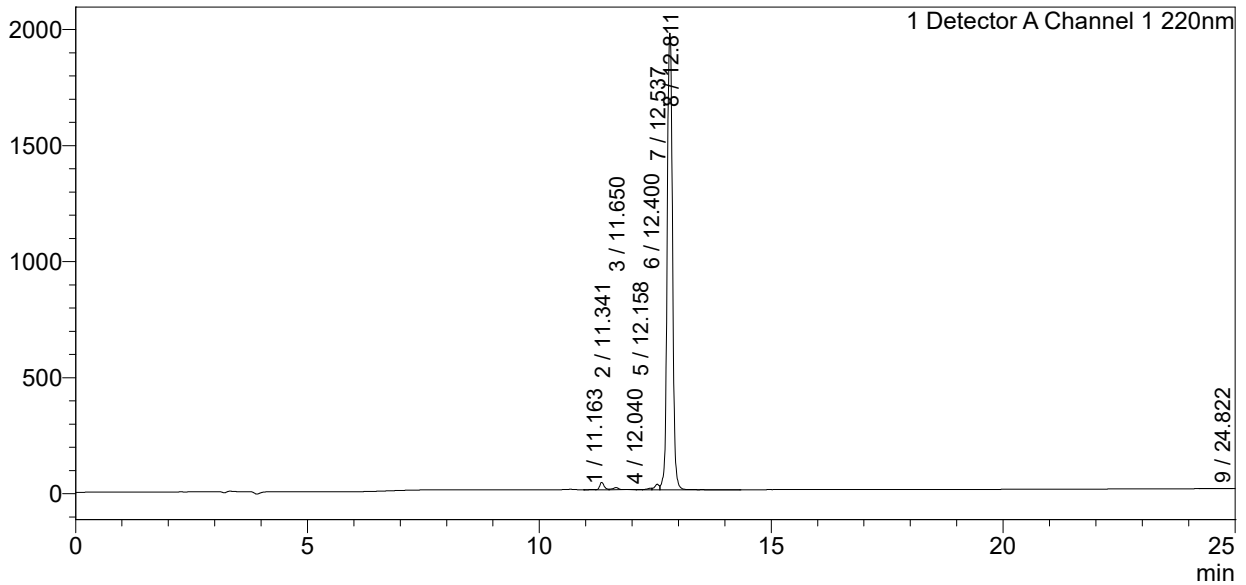

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.163	5712	719	0.035
2	11.341	208405	31801	1.279
3	11.650	78054	9484	0.479
4	12.040	3700	579	0.023
5	12.158	5025	781	0.031
6	12.400	42184	6423	0.259
7	12.537	163613	23710	1.004
8	12.811	15778877	1968297	96.832
9	24.822	9593	368	0.059
Total		16295164	2042164	100.000