

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E4689219I
 Time Processed :9:58:05 AM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

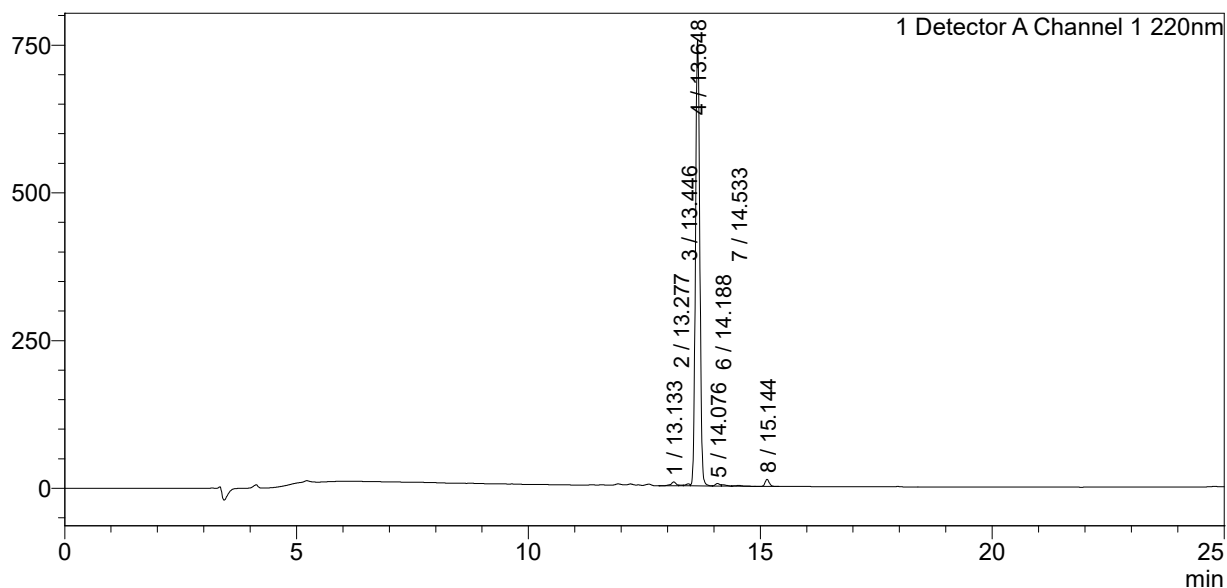

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.133	53572	6688	1.059
2	13.277	8609	1543	0.170
3	13.446	22630	3463	0.447
4	13.648	4842799	756227	95.740
5	14.076	28191	4236	0.557
6	14.188	14509	2137	0.287
7	14.533	12258	1050	0.242
8	15.144	75695	11975	1.496
Total		5058263	787320	100.000