

Sample Name :Bim BH3, Peptide IV
 Cat No. :RP20339
 Lot No. :E7981220L
 Time Processed :4:56:23 AM
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

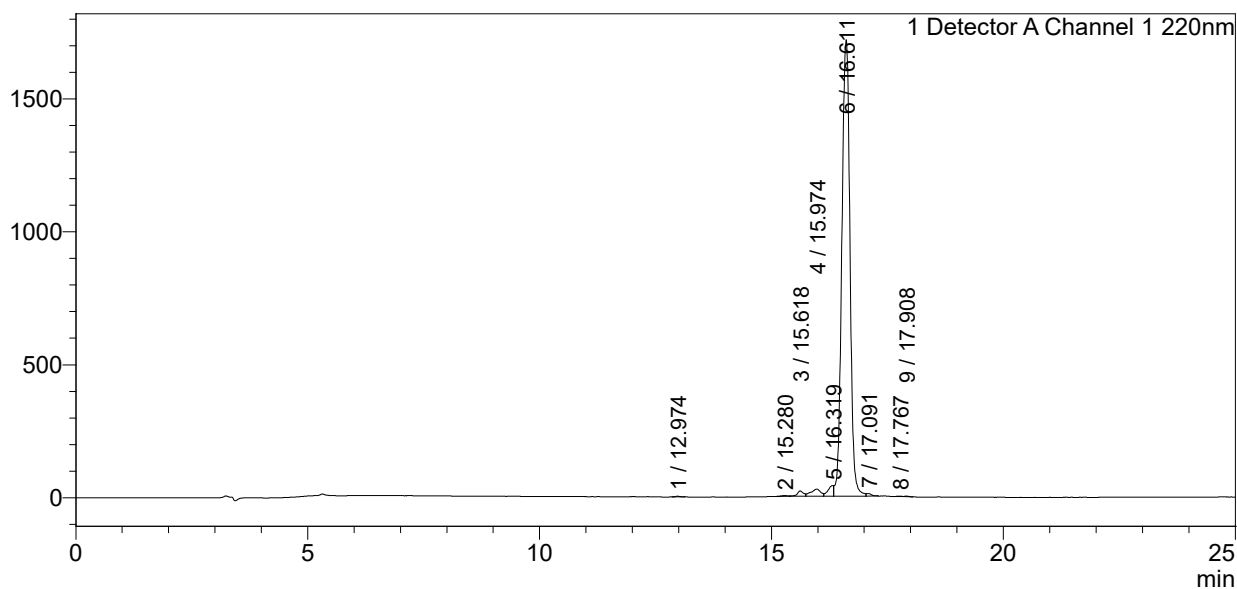

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.974	18710	2972	0.085
2	15.280	28688	3021	0.131
3	15.618	193516	20352	0.881
4	15.974	393733	26970	1.792
5	16.319	337897	40092	1.538
6	16.611	20910041	1716797	95.150
7	17.091	65686	9436	0.299
8	17.767	12760	1753	0.058
9	17.908	14851	2530	0.068
Total		21975882	1823922	100.000