

Sample Name:p53(17-26)
 Cat No. : RP20338
 Lot No. : E7069919J
 Time Processed: 1:16:18 AM
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

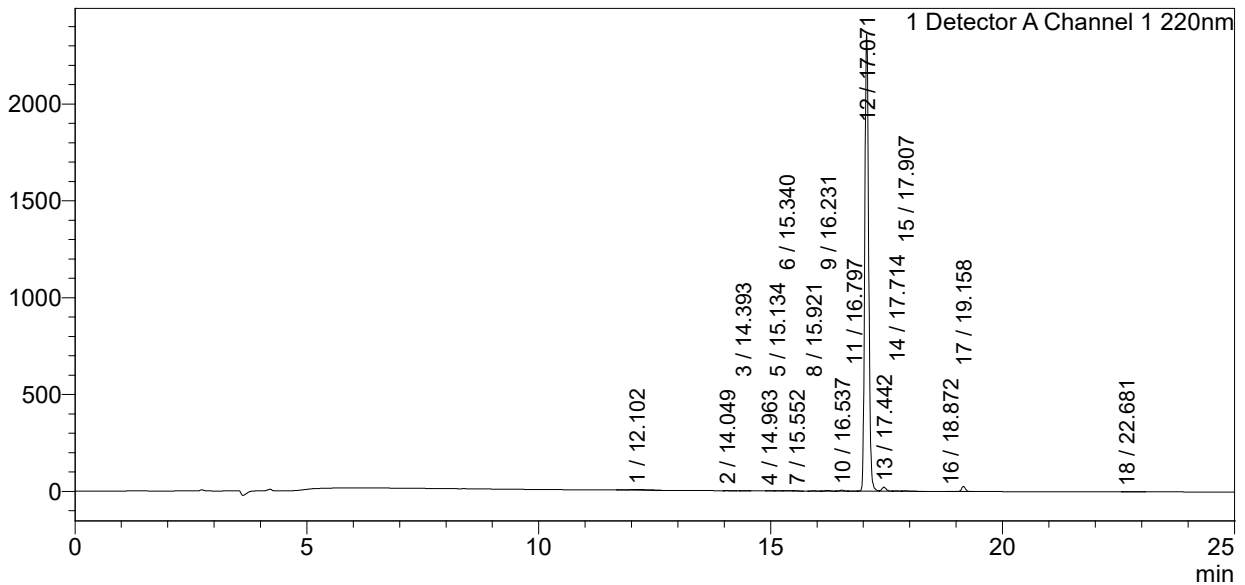

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.102	89878	2542	0.635
2	14.049	2627	511	0.019
3	14.393	1854	371	0.013
4	14.963	1175	249	0.008
5	15.134	1041	241	0.007
6	15.340	1215	195	0.009
7	15.552	1606	322	0.011
8	15.921	3021	375	0.021
9	16.231	21344	3566	0.151
10	16.537	27491	4787	0.194
11	16.797	1373	294	0.010
12	17.071	13689063	2359943	96.693
13	17.442	131924	20906	0.932
14	17.714	8816	1433	0.062

Peak#	Ret. Time	Area	Height	Area%
15	17.907	19283	1977	0.136
16	18.872	1352	225	0.010
17	19.158	152450	26451	1.077
18	22.681	1670	111	0.012
Total		14157184	2424499	100.000