

Sample Name :  $\beta$ -Endorphin, human  
 Cat. No. : RP11344  
 Lot. No. : E4000221F  
 Time Processed : 22:27:37  
 Month-Day-Year Processed : 06/18/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
45.00	Pumps	Pump A B.Conc	5
95.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010017

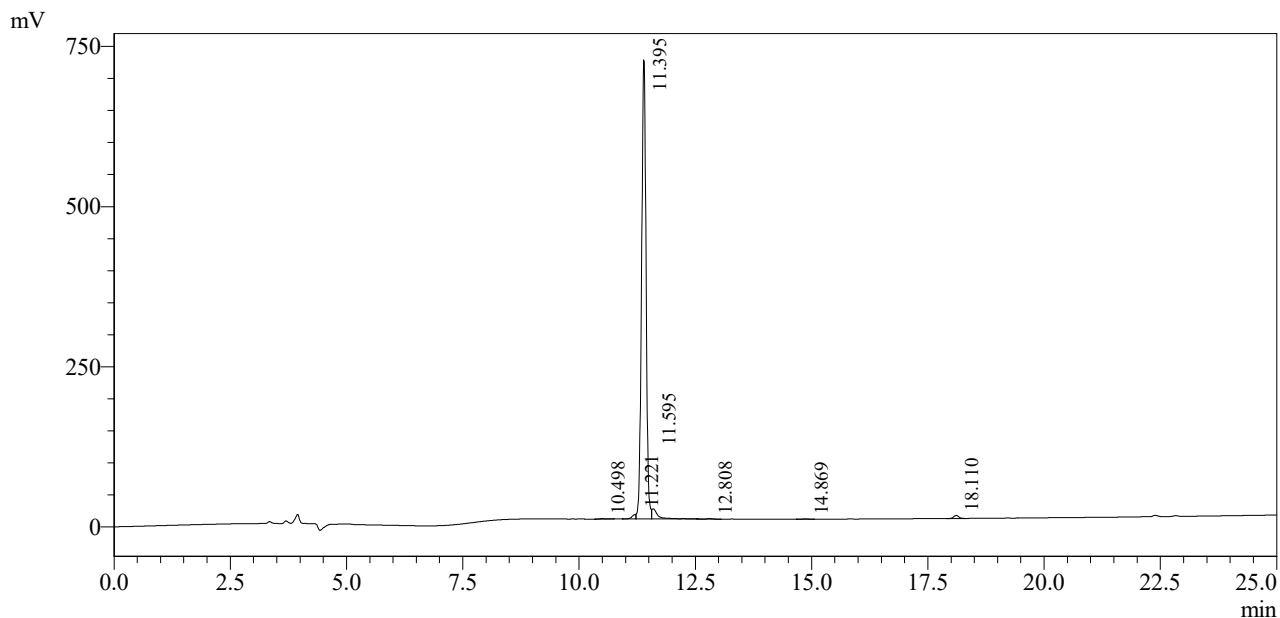

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.498	5086	732	0.101
2	11.221	42851	7138	0.848
3	11.395	4816931	716893	95.286
4	11.595	143488	15717	2.838
5	12.808	5349	867	0.106
6	14.869	6020	728	0.119
7	18.110	35518	4684	0.703
Total		5055242	746761	100.000