


Mass Spectrum

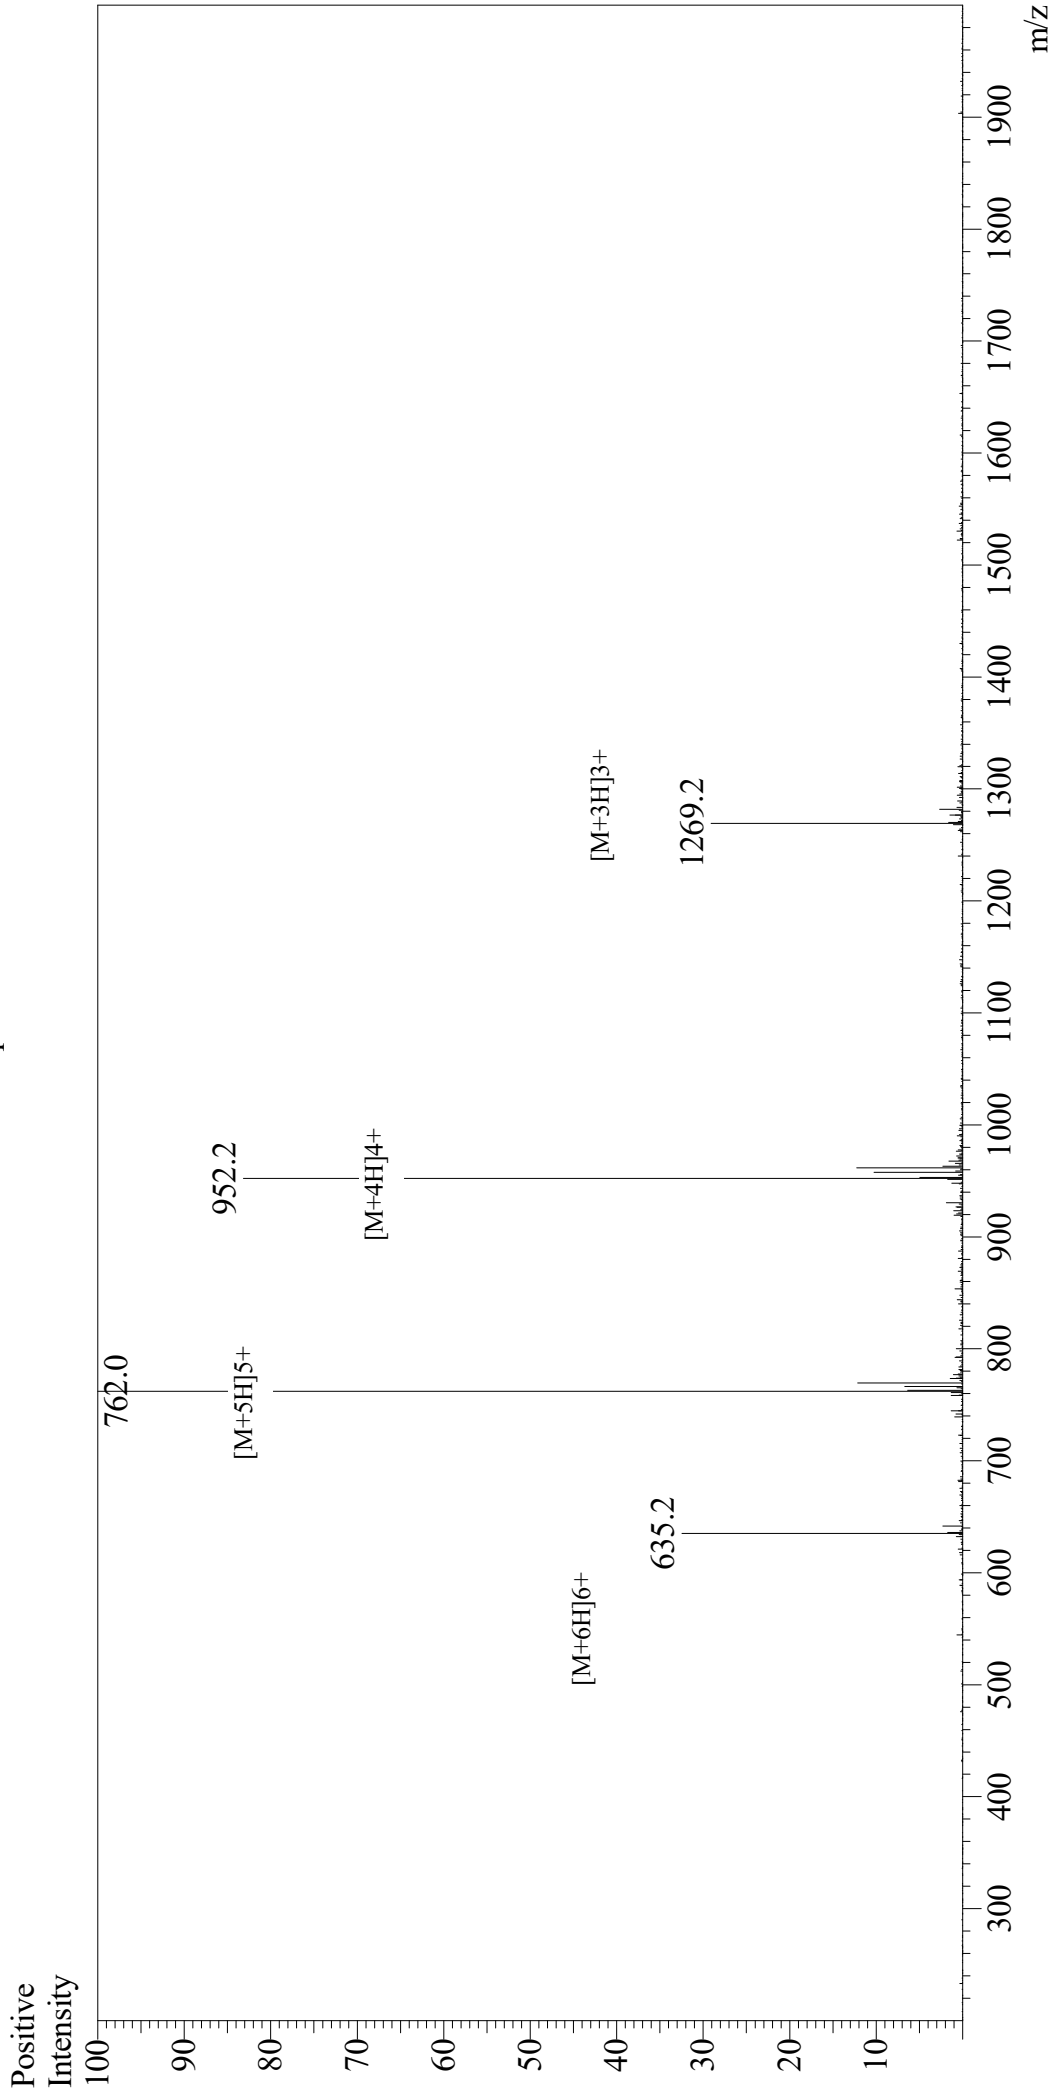

Sample Information

User : Gary
Month-Day Processed : 03/01/19
Time Processed : 02:44:07 PM
Injection Volume : 0.2
Sample Name : CGRP II, rat
Cat No. : RP11092
Lot No. : PE7941902
Theoretical MW : 3805.40
Observed MW : 3805.0

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH